

TECHNICAL DATA SHEET



bioauxilium

BETTER TOOLS. REAL DISCOVERIES.

THUNDER™ Phospho-c-Met (Y1234/Y1235) + Total c-Met TR-FRET Cell Signaling Assay Kit

CATALOG NUMBERS KIT-METPT-500
400 points for phospho c-MET and 100 points for total c-MET

Store at -80°C
For research use only.
Not for use in diagnostic procedures.

PRODUCT DESCRIPTION

This assay kit measures intracellular levels of **phospho-c-Met (Y1234/Y1235)** and **total c-MET** protein in cell lysates using a simple, rapid and sensitive immunoassay based on the homogeneous (no-wash) THUNDER™ TR-FRET technology. The kit is compatible with both adherent and suspension cells.

SPECIFICITY

This assay kit contains two specific and selective antibody pairs, one that recognizes **c-Met** phosphorylated at **Tyr1234** and **Tyr1235** and another that recognizes **total** (both phosphorylated and unphosphorylated) **c-MET**.

SPECIES REACTIVITY

Human (Swiss-Prot Acc.: P08581; Entrez-Gene Id: 4233).

Other species should be tested on a case-by-case basis.

TR-FRET ASSAY PRINCIPLE

The **Phospho-c-Met (Y1234/Y1235) + Total c-Met** assay kit is a homogeneous time-resolved Förster resonance energy transfer (TR-FRET) sandwich immunoassay (Figure 1). The THUNDER™ Cell Signaling assay workflow consists of 3 steps (Figure 2). Following cell treatment, cells are first lysed with the specific Lysis Buffer provided in the kit. Then **Phospho-c-Met (Y1234/Y1235)** and **Total c-Met** in the cell lysates are detected in separate wells with two pairs of fluorophore-labeled antibodies in a simple "add-incubate-measure" format (single-step reagent addition; no wash steps). For detection of the phosphorylated protein, one antibody is labeled with a donor fluorophore (Europium chelate; Eu-Ab1) and the second with a far-red acceptor fluorophore (FR-Ab2). The same approach is used for the second antibody pair detecting the total protein (Eu-Ab3 and FR-Ab4). The binding of the two matched labeled antibodies to distinct epitopes on the target protein (either **phospho-c-Met** or **total c-Met**) takes place in solution and brings the two dyes into close proximity. Excitation of the donor Europium chelate molecules with a flash lamp (320 or 340 nm) or a laser (337 nm) triggers a FRET from the donor to the acceptor molecules, which in turn emit a TR-FRET signal at 665 nm. Residual energy from the Eu chelate generates light at 615 nm. The signal at 665 nm is proportional to the concentration of **Phospho-c-Met (Y1234/Y1235)** and **Total c-Met** in the cell lysate. Data can be expressed as either the signal at 665 nm or the 665 nm/615 nm ratio.

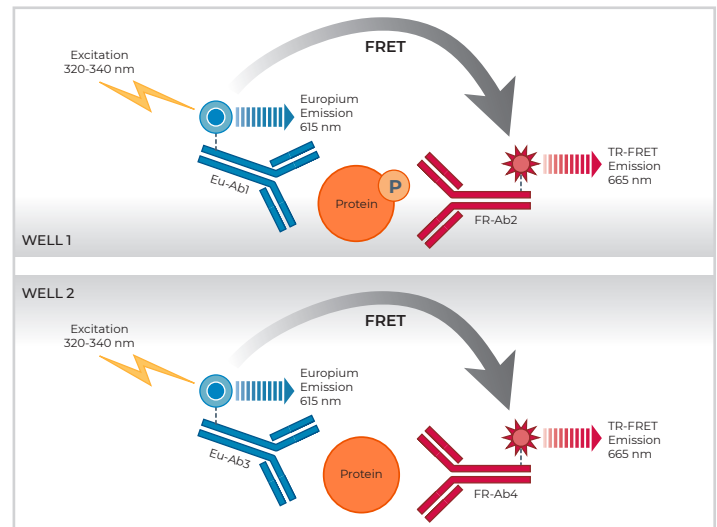


Fig. 1 Schematic representation of the TR-FRET cell signaling assay principle.

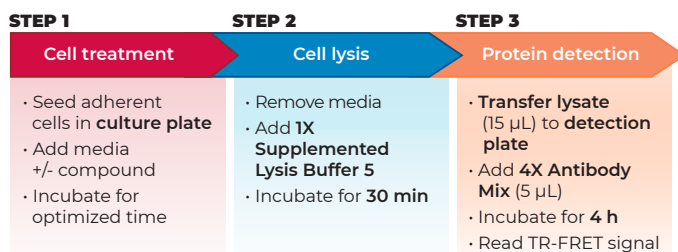


Figure 2 Assay workflow using the 2-plate (transfer) protocol.

KIT COMPONENTS

	500 points*
Eu-labeled phospho-c-Met (Y1234/Y1235) antibody (Eu-Ab1)	20 µL
Acceptor-labeled phospho-c-Met (Y1234/Y1235) antibody (FR-Ab2)	80 µL
Eu-labeled total-c-Met antibody (Eu-Ab3)	5 µL
Acceptor-labeled total-c-Met antibody (FR-Ab4)	20 µL
Lysis Buffer 5 (5X)	5 mL
Detection Buffer (10X)	250 µL
Positive control cell lysate	200 µL
Phosphatase Inhibitor Cocktail (100X)	250 µL

* The number of assay points is based on an assay volume of 20 µL in half-area 96-well or low-volume 384-well assay plates using the kit components at the recommended concentrations (refer to the User Manual).

TECHNICAL DATA SHEET


Phospho-c-Met (Y1234/Y1235) + Total c-Met

VALIDATION DATA

This assay kit has been validated for the relative quantification of phospho-c-Met (Y1234/1235) and total c-Met in HeLa and A431 cell lysates using the 2-plate assay protocol.


- Adherent cells were cultured overnight in a 96-well tissue culture plate (DMEM +10% FBS).
- Following cell treatment, the media was removed and cells were lysed with the 1X **Lysis Buffer 5** (50 μ L) supplemented with the phosphatase inhibitors sodium fluoride (1 mM), sodium orthovanadate (2 mM), cOmplete™, Mini, EDTA-free protease inhibitor cocktail (Roche), bpV(phen) (0.1 mg/mL) and PMSF (1 mM).
- Following a **30-min** incubation at room temperature (RT) on an orbital shaker (400 rpm), lysates (15 μ L) were then transferred to a 384-well assay plate followed by addition to separate wells of either the labeled antibodies Eu-Ab1 and FR-Ab2 (5 μ L) for detection of phospho-c-Met (Y1234/1235) or Eu-Ab3 and FR-Ab4 (5 μ L) for detection of total c-Met.
- The plate was incubated at RT for **4 hours** and the TR-FRET signal was recorded at 665 and 615 nm (EnVision®; lamp excitation).

STIMULATION OF PHOSPHO-C-MET (Y1234/Y1235) IN A431 CELLS

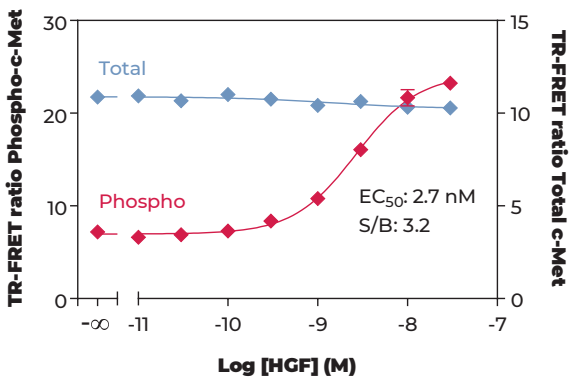


A431 cells (50,000 cells/well; in triplicate) were incubated with serial dilutions of HGF for 10 min at RT. Data show that treatment of A431 cells with HGF stimulates phosphorylation of c-Met at Y1234/Y1235, but does not affect the levels of total c-Met.

INHIBITION OF PHOSPHO-C-MET (Y1234/Y1235) IN HELA CELLS

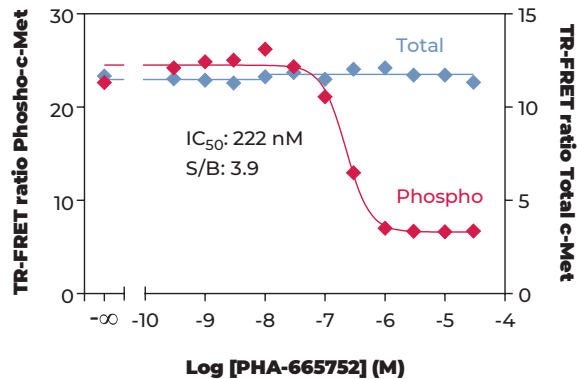

HeLa cells (50,000 cells/well; in triplicate) were incubated with serial dilutions of PHA-665752 for 60 min at RT. Cells were then stimulated with 10 nM of HGF for 10 min at RT. Data show that treatment of HeLa cells with PHA-665752 inhibits phosphorylation of c-Met at Y1234/Y1235 by HGF, but does not affect the levels of total c-Met.

HELA CONTROL LYSATE TITRATION (QC TEST) PHOSPHO-C-MET (Y1234/1235)

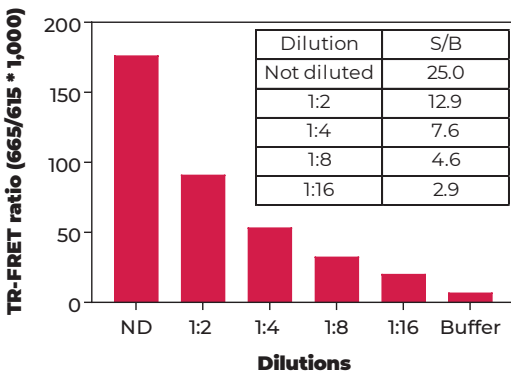

Quality Control: the Phospho-c-Met (Y1234/Y1235) + Total c-Met assay kit is routinely tested against pervanadate-treated HeLa lysates. HeLa cells were cultured in a T175 flask to 90% confluence and stimulated with 1 mM of pervanadate for 15 min at 37°C. Following cell lysis using 4 mL of 1X Lysis Buffer 5, lysates were serially diluted with 1X Lysis Buffer 5 and tested in triplicate and in separate wells for phospho-c-Met (Y1234/Y1235) and total c-Met. Data show a linear relationship between lysate dilutions and TR-FRET ratio values.

HELA CONTROL LYSATE TITRATION (QC TEST) TOTAL C-MET

