


VALIDATION DATA

This assay kit has been validated for the relative quantification of phospho-SLP-76 (S376) in Jurkat cell lysates using the 2 plate assay protocol.

- Non-adherent cells were cultured in RPMI+10% FBS before being centrifuged and resuspended at the desired density in RPMI without serum.
- Following cell treatment, cells were lysed with the 5X **Lysis Buffer 1** (to a final concentration of 1X) supplemented with the phosphatase inhibitors sodium fluoride (5 mM) and sodium orthovanadate (10 mM).


- Following a **30-min** incubation at room temperature (RT) on an orbital shaker (400 rpm), lysates (15 μ L) were then transferred to a 384-well assay plate followed by addition of the labeled antibodies Eu-Ab1 and FR-Ab2 (5 μ L) for detection of phospho-SLP-76 (S376).
- The plate was incubated at RT for **18 hours** and the TR-FRET signal was recorded at 665 and 615 nm (EnVision®; lamp excitation).

STIMULATION OF PHOSPHO-SLP-76 (S376) IN JURKAT CELLS

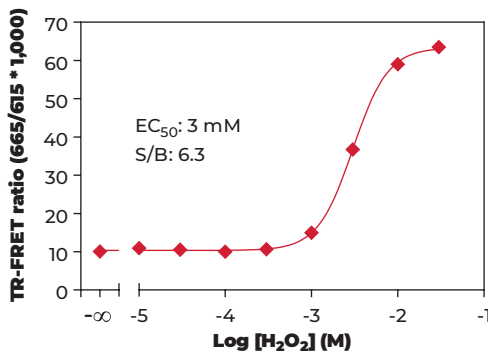


Jurkat cells (400,000 cells/well in triplicate) plated in a 96-well tissue culture plate were incubated with serial dilutions of H₂O₂ for 15 min at RT. Data show that treatment of Jurkat cells with H₂O₂ stimulates phosphorylation of SLP-76 at S376.

Z'-FACTOR DETERMINATION IN JURKAT CELLS

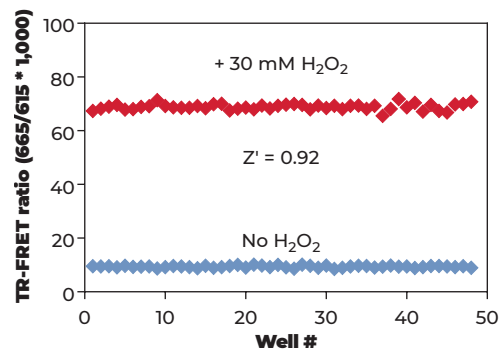


Jurkat cells (400,000 cells/well) were incubated without or with 30 mM H₂O₂ for 15 min at RT. The Z' factor value was determined using a total of 48 wells for each treatment group. The Z'-factor value of 0.92 indicates that the assay is robust and suitable for HTS.

JURKAT CONTROL LYSATE TITRATION (QC TEST)

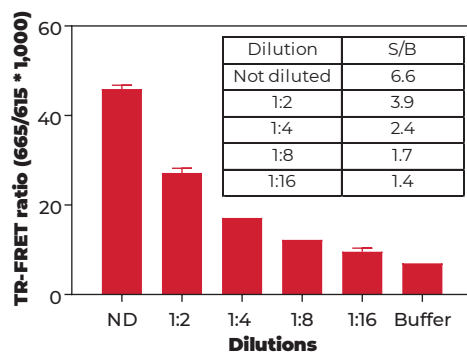

Quality Control: the Phospho-SLP-76 (S376) assay kit is routinely tested against H₂O₂ treated Jurkat lysates. Jurkat cells were cultured, centrifuged, resuspended at 20 million cells/mL and stimulated with 30 mM of H₂O₂ for 15 min at RT. Following cell lysis with 5X Lysis Buffer 1 (final concentration: 1X), lysates were serially diluted with 1X Lysis Buffer 1 and tested in triplicate. Data show a linear relationship between lysate dilutions and TR-FRET ratio values.

ALL-IN-ONE-WELL PHOSPHO-SLP-76 (S376) ASSAY

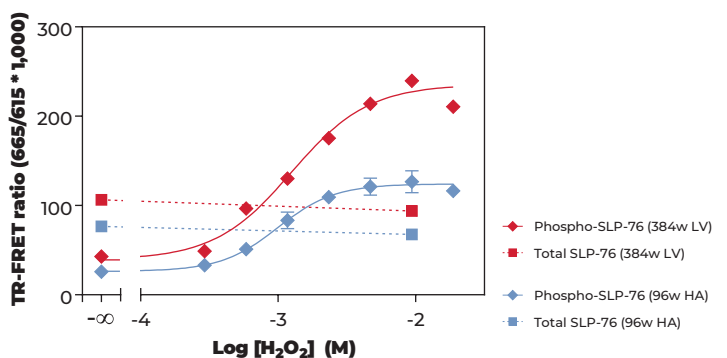


Jurkat cells (100,000 cells/well in triplicate) were plated in 8 μ L in either a low volume (LV) 384-well assay plate or a half-area (HA) 96-well assay plate and immediately incubated with 4 μ L of H₂O₂ for 15 min at RT. Cells were then lysed with 3 μ L of 5X supplemented Lysis Buffer 1. Following a 30-min incubation at RT on an orbital shaker (400 rpm), 5 μ L of labeled antibodies Eu-Ab1 and FR-Ab2 were added directly to the lysate for detection of phospho-SLP-76 (S376) in the same well, without a transfer step (1-plate assay protocol). Data show that stimulation of phospho-SLP-76 (S376) by H₂O₂ in Jurkat cells can be detected using the 1-plate assay protocol in both LV 384 and HA 96-well plates.




KIT BENCHMARKING – COMPARISON TO OTHER TR-FRET TECHNOLOGIES

As part of assay validation, the THUNDER™ Phospho-SLP-76 (S376) Assay Kit was benchmarked against two competitive TR-FRET assay technologies (Companies A and B). Specifically, the 3 different assays were compared side-by-side for their capacity to detect phospho-SLP-76 (S376) stimulation upon Jurkat cell treatment with H₂O₂ using the 2-plate assay protocol. All reagents were prepared according to each manufacturer's recommendations. Following cell treatment, cells were lysed with the corresponding kit's 1X Lysis Buffer supplemented with phosphatase inhibitors. Lysates were then tested on the same 384-well assay plate and according to the corresponding kit's standard protocol. The plate was read on an EnVision® (lamp excitation) following 4 hours (THUNDER™ and Company B) or 18 hours (Company A). Data show that the 3 TR-FRET assays exhibited comparable sensitivity (EC₅₀ values). The Company B assay showed a slightly higher S/B ratio.

THUNDER™ PHOSPHO-SLP-76 (S376) ASSAY KIT

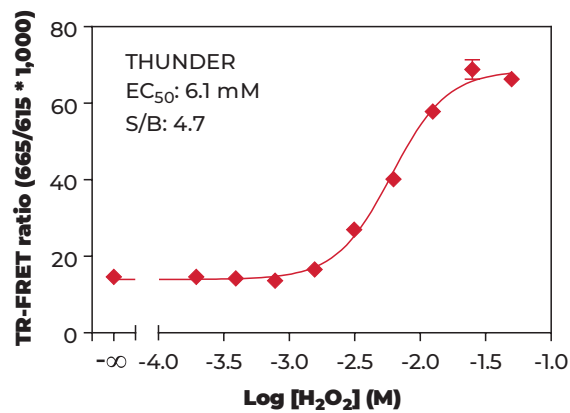

COMPANY A PHOSPHO-SLP-76 (S376) ASSAY KIT

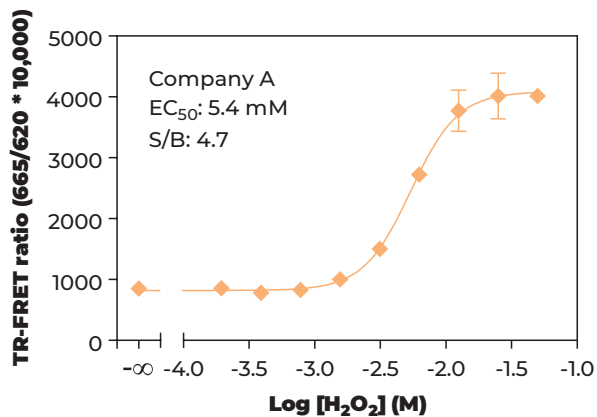

COMPANY B PHOSPHO-SLP-76 (S376) ASSAY KIT

